

Diazotization Method¹

Method 10237

0.6 to 6.0 mg/L NO₂⁻-N or 2.0 to 20.0 mg/L NO₂⁻ (HR)

TNTplus 840

Scope and application: For wastewater, drinking water, surface water and process water,

¹ Adapted from Standard Methods for the Examination of Water and Wastewater.



Test preparation

Instrument-specific information

Table 1 shows all of the instruments that have the program for this test. The table also shows the adapter and light shield requirements for the applicable instruments that can use TNTplus vials.

To use the table, select an instrument, then read across to find the applicable information for this test.

Table 1 Instrument-specific information for TNTplus vials

Instrument	Adapters	Light shield
DR6000, DR5000	—	—
DR3900	—	LZV849
DR3800, DR2800	—	LZV646
DR1900	9609900 or 9609800 (A)	—

Before starting

DR3900, DR3800, DR2800: Install the light shield in Cell Compartment #2 before this test is started.

Review the safety information and the expiration date on the package.

The recommended sample pH is 3–10.

The recommended temperature for samples and reagents is 15–25 °C (59–77 °F).

The recommended temperature for reagent storage is 15–25 °C (59–77 °F).

DR1900: Go to All Programs>LCK or TNTplus Methods>Options to select the TNTplus number for the test. Other instruments automatically select the method from the barcode on the vial.

Review the Safety Data Sheets (MSDS/SDS) for the chemicals that are used. Use the recommended personal protective equipment.

Dispose of reacted solutions according to local, state and federal regulations. Refer to the Safety Data Sheets for disposal information for unused reagents. Refer to the environmental, health and safety staff for your facility and/or local regulatory agencies for further disposal information.

Items to collect


Description	Quantity
Nitrite HR TNTplus Reagent Set	1
Pipet, adjustable volume, 0.1–1.0 mL	1
Pipet tips, for 0.1–1.0 mL pipet	1

Refer to [Consumables and replacement items](#) on page 4 for order information.

Sample collection and storage

- Collect samples in clean glass or plastic bottles.
- To preserve samples for later analysis, keep the samples at or below 6 °C (43 °F) for up to 48 hours.
- Let the sample temperature increase to room temperature before analysis.


Test procedure

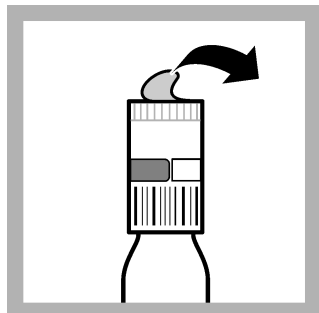


1. Carefully remove the lid from the DosiCap™ Zip cap. Remove the cap from the test vial.



2. Use a pipet to add 0.2 mL of sample to the test vial. Immediately continue to the next step.

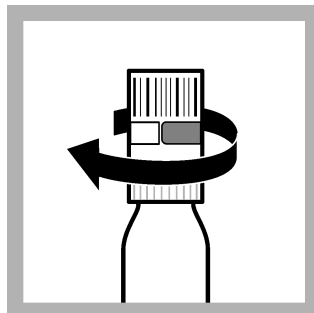


3. Turn the DosiCap Zip over so that the reagent side goes on the test vial. Tighten the cap on the vial.

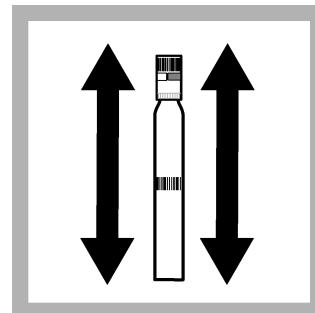


4. Shake the vial 2–3 times to dissolve the reagent in the cap. Look through the open end of the DosiCap to make sure that the reagent has dissolved.




5. Start the reaction time of 10 minutes.

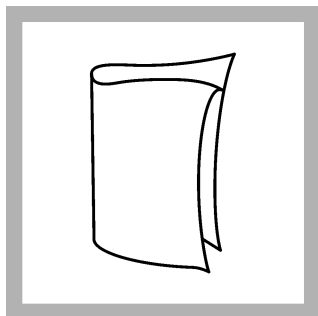

6. When the timer expires, clean the vial.

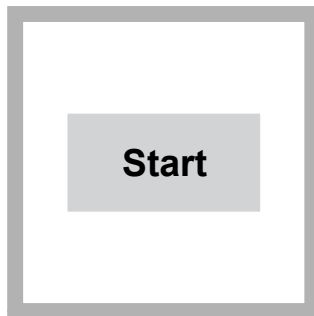

7. DR1900 only: Select program 840. Refer to [Before starting](#) on page 1.

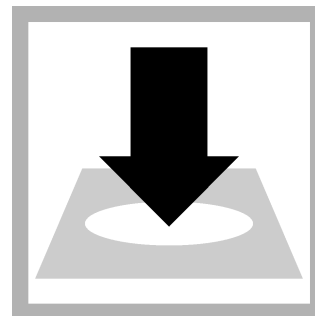

8. Insert the vial into the cell holder. DR1900 only: Push **READ**. Results show in mg/L NO₂⁻-N.

Reagent blank correction

For the best results, measure the reagent blank value for each new lot of reagent. Replace the sample with deionized water in the test procedure to determine the reagent blank value. Subtract the reagent blank value from the sample results automatically with the reagent blank adjust option. Measure the reagent blank value when a new lot of reagent is used.

1. Use deionized water as the sample in the test procedure to measure the reagent blank value.
2. Set the reagent blank function to on. The measured reagent blank value is shown.
3. Accept the blank value. The reagent blank value is then subtracted from all results until the reagent blank function is set to off or a different method is selected.

Note: As an alternative, record or enter the reagent blank value at a different time. Push the highlighted reagent blank box and use the keypad to enter the value.

Sample blanks

Samples with color or turbidity can cause high results. Samples without color or turbidity do not require sample blanks. To adjust for color or turbidity, use the steps that follow to find the sample blank.

1. Do the test procedure, but do not remove the foil lid from the vial.
2. Put the cap on the vial.
3. Subtract the value from the final procedure step from the initial sample value to get the corrected sample concentration.

Interferences

Table 2 that the ions were individually examined to the given concentrations and do not cause interference. No cumulative effects or influences of other ions were found.

Chromium (VI) ions interfere with the determination. Copper (II) ions interfere with the determination even at concentrations below 1 mg/L.

Table 2 Interfering substances

Interfering substance	Interference level
Sn ⁴⁺	10 mg/L
Fe ²⁺ , Fe ³⁺ , Ni ²⁺ , Ag ⁺	20 mg/L
Co ²⁺ , Zn ²⁺ , Cd ²⁺ , Mn ²⁺	50 mg/L
Cr ³⁺ , Hg ²⁺	100 mg/L
Mg ²⁺	200 mg/L
NH ₄ ⁺ , PO ₄ ³⁻	1000 mg/L
K ⁺ , NO ₃ ⁻ , Ca ²⁺ , Cl ⁻	2000 mg/L
SO ₄ ²⁻	4000 mg/L

Accuracy check

Standard solution method

Use the standard solution method to validate the test procedure, the reagents and the instrument.

Items to collect:

- 3.0-mg/L NO₂⁻-N Standard Solution¹

1. Use the test procedure to measure the concentration of the standard solution.
2. Compare the expected result to the actual result.

Method performance

The method performance data that follows was derived from laboratory tests that were measured on a spectrophotometer during ideal test conditions. Users can get different results under different test conditions.

Program	Standard	Precision (95% confidence interval)	Sensitivity Concentration change per 0.010 Abs change
barcode	3.0 mg/L NO ₂ ⁻ -N	2.94–3.06 mg/L NO ₂ ⁻ -N	0.05 mg/L NO ₂ ⁻ -N

¹ Nitrite standard solutions are difficult to prepare. Use the instructions in Standard Methods for the Examination of Water and Wastewater, Method 4500—NO₂⁻-B.

Summary of Method

Nitrite in the sample reacts with a primary aromatic amine in acidic solution to form a diazonium salt. This couples with an aromatic compound to form a complex with color that is directly proportional to the amount of nitrite in the sample. The measurement wavelength is 515 nm.

Consumables and replacement items

Required reagents

Description	Quantity/Test	Unit	Item no.
Nitrite HR TNTplus Reagent Set	1	25/pkg	TNT840

Required apparatus

Description	Quantity/test	Unit	Item no.
Pipet, adjustable volume, 0.1–1.0 mL	1	each	BBP078
Pipet tips, for 0.1–1.0 mL pipet	2	100/pkg	BBP079
Light shield, DR3800, DR2800, DR2700	1	each	LZV646
Light shield, DR3900	1	each	LZV849

Recommended standards

Description	Unit	Item no.
Sodium Nitrite, ACS	454 g	245201

Optional reagents and apparatus

Description	Unit	Item no.
Sampling bottle with cap, low density polyethylene, 500 mL	12/pkg	2087079
Test tube rack, polyethylene, for 13-mm OD vials, 90 holes	each	2497900
Water, deionized	4 L	27256



FOR TECHNICAL ASSISTANCE, PRICE INFORMATION AND ORDERING:
In the U.S.A. – Call toll-free 800-227-4224
Outside the U.S.A. – Contact the HACH office or distributor serving you.
On the Worldwide Web – www.hach.com; E-mail – techhelp@hach.com

HACH COMPANY
WORLD HEADQUARTERS
Telephone: (970) 669-3050
FAX: (970) 669-2932