

Hach BioTector B3500dw TOC Analyser

Applications

- Drinking water



Maximum uptime and reliability for TOC analysis in drinking water applications

The Hach® BioTector B3500dw uses unique technology that only requires scheduled maintenance every 6 months and delivers 99.86% uptime ensuring total confidence in your TOC measurement.

Rock solid reliability

With unique, EPA method approved Two Stage Advanced Oxidation Technology, the self-cleaning sample reactor of B3500dw delivers maximum reliability.

Lowest cost of ownership

With its 99.86% uptime, semi-annual maintenance and reagent replenishment is all that is needed.

Secure your source water

TSAO technology analyses organics in your source that are invisible to scanning UV technologies.

Technical Data*

Parameter	TOC (NPOC), TIC, % TOC removal (with 2 streams) and COD, BOD after correlation
Measurement method	Infrared measurement of CO ₂ after oxidation (DIN EN 1484:1997-08, ISO 8245:1999-03, EPA 415.1)
Oxidation method	Unique Two-Stage Advanced Oxidation Process (TSAO) using Hydroxyl Radicals, Hach Company method 10261 (EPA approved for drinking water)
Measuring range	0 - 25 mg/L C
Multi-Stream	1 stream
Repeatability	±3% of reading or ±0.03 mg/L, whichever is greater; Lower Limit of detection LOD = 0.06 mg/L
Cycle time	From 5.5 minutes, depending on range and application
Communication: digital	Modbus RTU, Modbus TCP/IP & Profibus (when the Profibus option is selected, the digital output signals are sent through the Profibus converter with its specific communication protocol)

Sample inlet temperature	0 - 60 °C
Ambient temperature	5 - 45 °C
Humidity	5 - 85 % (non-condensing)
Particle size	Up to 100 µm
Data storage	Previous 9999 reaction data Previous 99 fault events
Display	High contrast 40 character x 16 line backlit LCD with LED backlight
User interface	Microcontroller with membrane keyboard
Power requirements (Voltage)	120/230 V AC
Power requirements (Hz)	50/60 Hz
Service interval	6 months service intervals
Dimensions (H x W x D)	750 mm x 500 mm x 320 mm
Weight	46 kg

*Subject to change without notice.

Principle of Operation

TIC

Acid is added to lower the pH so that inorganic carbon is sparged off as CO₂. This is measured to ensure Total Inorganic Carbon (TIC) is not carried over into the TOC.

Oxidation

BioTector's unique oxidation method (TSAO) achieves total and complete oxidation of the sample, including organic carbon to CO₂. TSAO utilises hydroxyl radicals generated within the analyser by combining oxygen, which passes through the ozone generator, with sodium hydroxide.


TOC

To remove CO₂ from the oxidised sample, the pH of the sample is lowered again. The CO₂ is sparged and measured by the specially developed NDIR CO₂ analyser. The result is displayed as Total Organic Carbon (TOC).




Dimensions


Front view

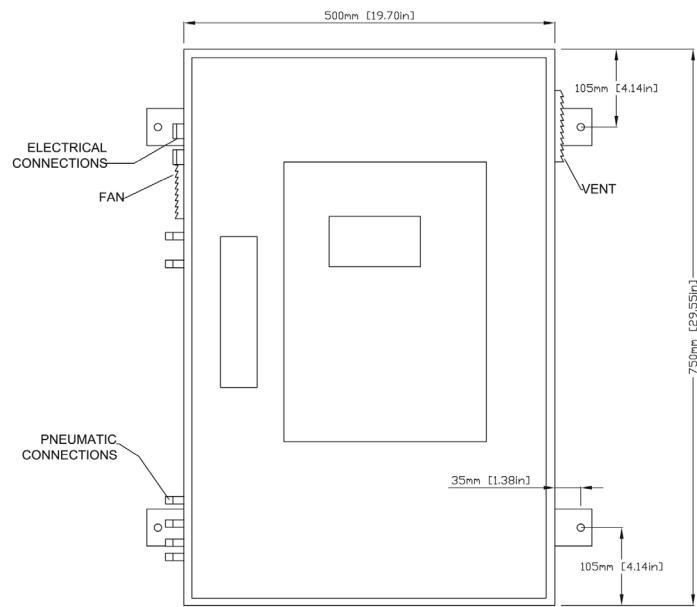

Side view

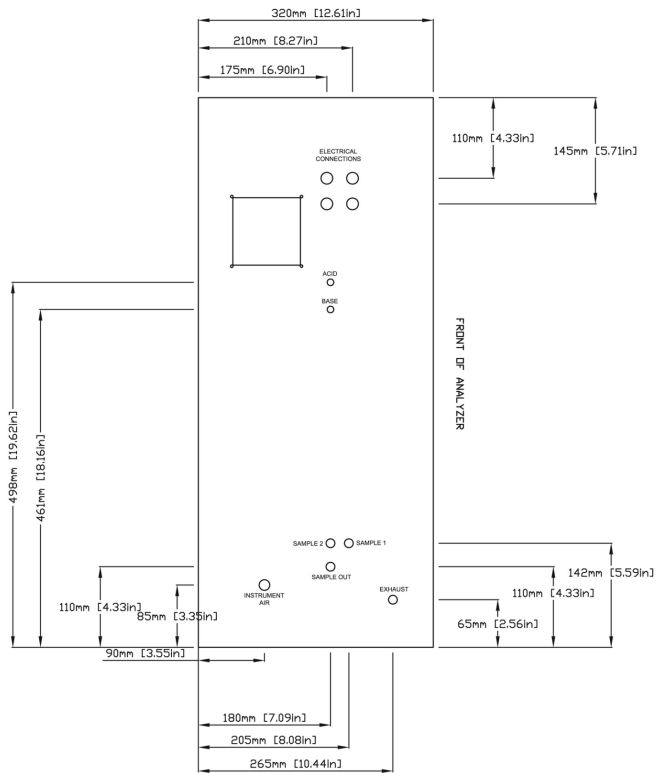

Top view

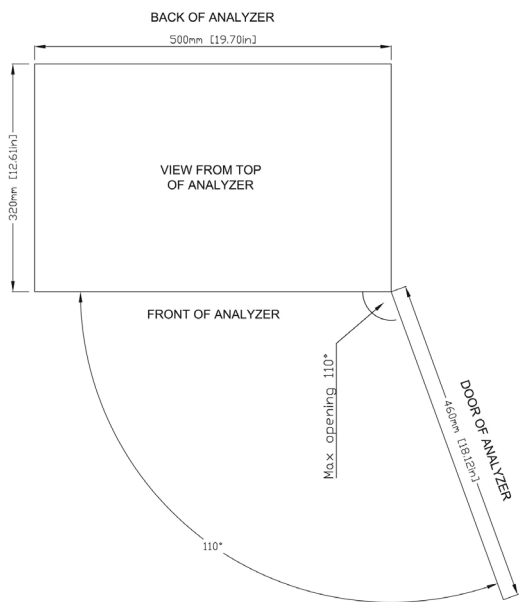

Panel detail



Order Information

Instruments

DWBCAA152AAA2 Hach BioTector B3500dw Online TOC analyser, 0 - 25 mg/L C, 1 stream, 230 V AC

DWBCAA152AAC2 Hach BioTector B3500dw Online TOC analyser, 0 - 25 mg/L C, 2 streams, 230 V AC

There are additional options available. Please contact Hach for more details.

Accessories

19-COM-160 BioTector compressor 115 V / 60 Hz

19-COM-250 BioTector compressor 230 V / 50 Hz

10-SMC-001 Air supply filter pack

19-KIT-123 Six months spare part kit for BioTector B3500

Reagents

2038062 BioTector reagent, 4.0 N NaOH

2038162 BioTector reagent, 6.0 N sulfuric acid with Mn catalyst

Hach Service Protects Your Investment

With Hach Service, you have a global partner who understands your needs and cares about delivering timely, high-quality service you can trust. Our Service Team brings unique expertise to help you maximise instrument uptime, ensure data integrity, maintain operational stability, and reduce compliance risk.