

15–150 mg/L  $\text{NO}_3^-$ -N or 66–664 mg/L  $\text{NO}_3^-$  High Range

TNTplus<sup>®</sup> 838—Method 10206

**Scope and application:** For wastewater (beware of interferences), drinking water, raw water, surface water, soils, substrates and nutrient solution.



## Test preparation

### Reagent storage

Storage temperature: 15–25 °C (59–77 °F)

### pH/Temperature

The pH of the water sample must be between pH 3–10.

The temperature of the water sample and reagents must be between 20–24 °C (68–75 °F).

### Before starting

**In case of not working at the correct recommended temperature an incorrect result may be obtained.**

Not more than **3 hours** should elapse between sampling and analysis. **Store in a cool place!**


The method is applicable for DR1900, DR3900 and DR6000 only.

Review safety information and expiration date on the package.


Review the Safety Data Sheets (MSDS/SDS) for the chemicals that are used. Use the recommended personal protective equipment.

Dispose of reacted solutions according to local, state and federal regulations. Refer to the Safety Data Sheets for disposal information for unused reagents. Refer to the environmental, health and safety staff for your facility and/or local regulatory agencies for further disposal information.


### Procedure

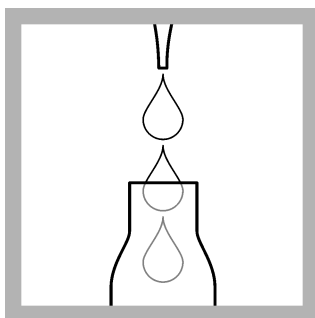


1. Slowly pipet 0.1 mL sample.

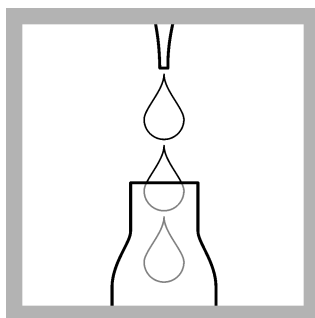

2. Slowly pipet 1.0 mL solution A.

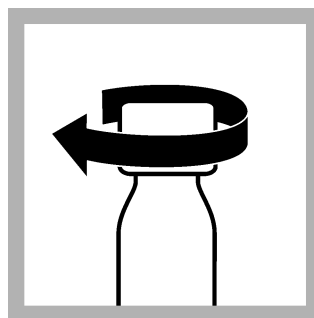


3. Close the vial.

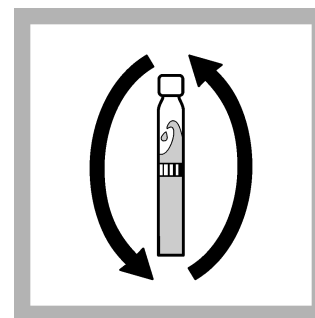


4. Invert 2–3 x until **no more streaks** can be seen.



5. Wait **15 minutes**.

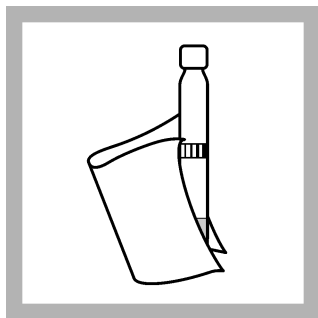

6. Thoroughly clean the outside of the vial.

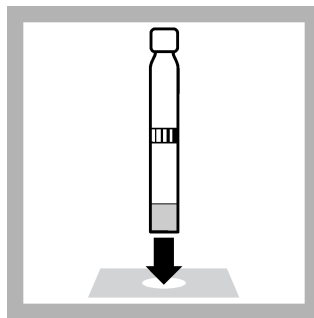

7. Insert the vial into the cell holder.  
DR1900: Go to LCK/TNTplus methods. Select the test, push **READ**.

## Interferences

The ions listed in the table have been individually checked against the given concentrations and do not cause interference. The cumulative effects and the influence of other ions have not been determined.

High loads of oxidizable organic substances (COD) cause the reagent to change color and to give high-bias results. The test can only be used for waste water analyses if the COD is less than 2000 mg/L.

The measurement results must be subjected to plausibility checks (dilute and/or spike the sample).

### Removal of Interferences

Nitrite concentrations of more than 5.0 mg/L interfere (high-bias results) and can be removed by the addition of a spatula-tip full of amidosulphonic acid. The chloride can be precipitated out as silver chloride by adding silver sulphate. High calcium concentrations cause turbidity. This interferes with the determination but can be prevented by adding a spatula-tip full of EDTA to the sample.

Interference level	Interfering substance
5000 mg/L	SO <sub>4</sub> <sup>2-</sup>
2000 mg/L	COD, K <sup>+</sup> , Na <sup>+</sup> , PO <sub>4</sub> <sup>3-</sup>
500 mg/L	Cl <sup>-</sup> , Ca <sup>2+</sup>
100 mg/L	Mg <sup>2+</sup> , Ag <sup>+</sup> , NH <sub>4</sub> <sup>+</sup>
50 mg/L	Co <sup>2+</sup> , Fe <sup>2+</sup> , Fe <sup>3+</sup> , Zn <sup>2+</sup> , Cu <sup>2+</sup> , Cd <sup>2+</sup> , Pb <sup>2+</sup> , Ni <sup>2+</sup>
5 mg/L	NO <sub>2</sub> <sup>-</sup> , Cr <sup>6+</sup>

## Summary of method

Nitrate ions in solutions containing sulphuric and phosphoric acids react with 2,6-dimethylphenol to form 4-nitro-2,6-dimethylphenol.

**TNT**  **plus**<sup>®</sup>



FOR TECHNICAL ASSISTANCE, PRICE INFORMATION AND ORDERING:  
In the U.S.A. – Call toll-free 800-227-4224  
Outside the U.S.A. – Contact the HACH office or distributor serving you.  
On the Worldwide Web – [www.hach.com](http://www.hach.com); E-mail – [techhelp@hach.com](mailto:techhelp@hach.com)

HACH COMPANY  
WORLD HEADQUARTERS  
Telephone: (970) 669-3050  
FAX: (970) 669-2932