Quality certificate

Technical data for cuvette test APC314

Sensitivity	- 0.004 Abs./(mg/L)
Ordinate intersect	0.804 Abs.
Residual standard deviation	0.0047 Abs.
Method variation coefficient	1.47 %
Method standard deviation	1.2 mg/L
Confidence interval (95%)	± 2.9 mg/L


The technical data for cuvette test APC314 were determined in conformity with ISO 8466-1 and DIN 38402 A51 „Calibration of analysis methods“.

The series of the smallest and largest calibration standards exhibit normal distribution and are outlier- and trend-free.
The calibration gives a linear function.

Technical data in conformity with DIN 32645

Detection limit	3.4 mg/L
Quantitation limit	10.2 mg/L

The detection and the quantitation limits were determined in conformity with DIN 32645.

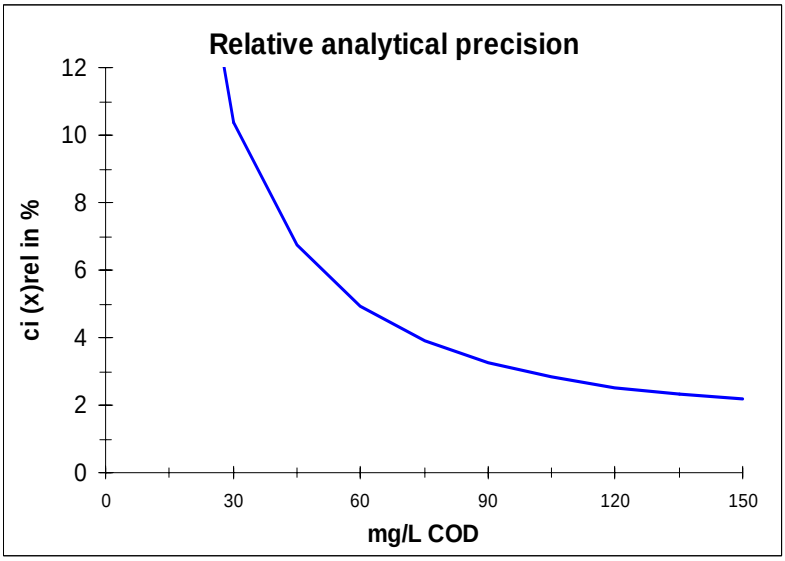

Result	Confidence interval (95%)
30 mg/L	± 3.1 mg/L
60 mg/L	± 3.0 mg/L
90 mg/L	± 2.9 mg/L
120 mg/L	± 3.0 mg/L
150 mg/L	± 3.2 mg/L

HACH LANGE GmbH

BU Lab Application
Dr. Ralf Kloos

HACH LANGE
UNITED FOR WATER QUALITY

HACH LANGE GmbH
Willstätterstraße 11
D-40549 Düsseldorf
Tel.+49 (0)211-52 88-320
Fax+49 (0)211-52 88-143
Kundenservice@hach-lange.de
www.hach-lange.de