Maintenance Schedule

FILTRAX *eco*

DOC273.52.90177.Mai09_1A

Number: Place of sampling:

Installation Date: by:

Inspection and Maintenance as part of the

Service Contract

Maintenance by the

User

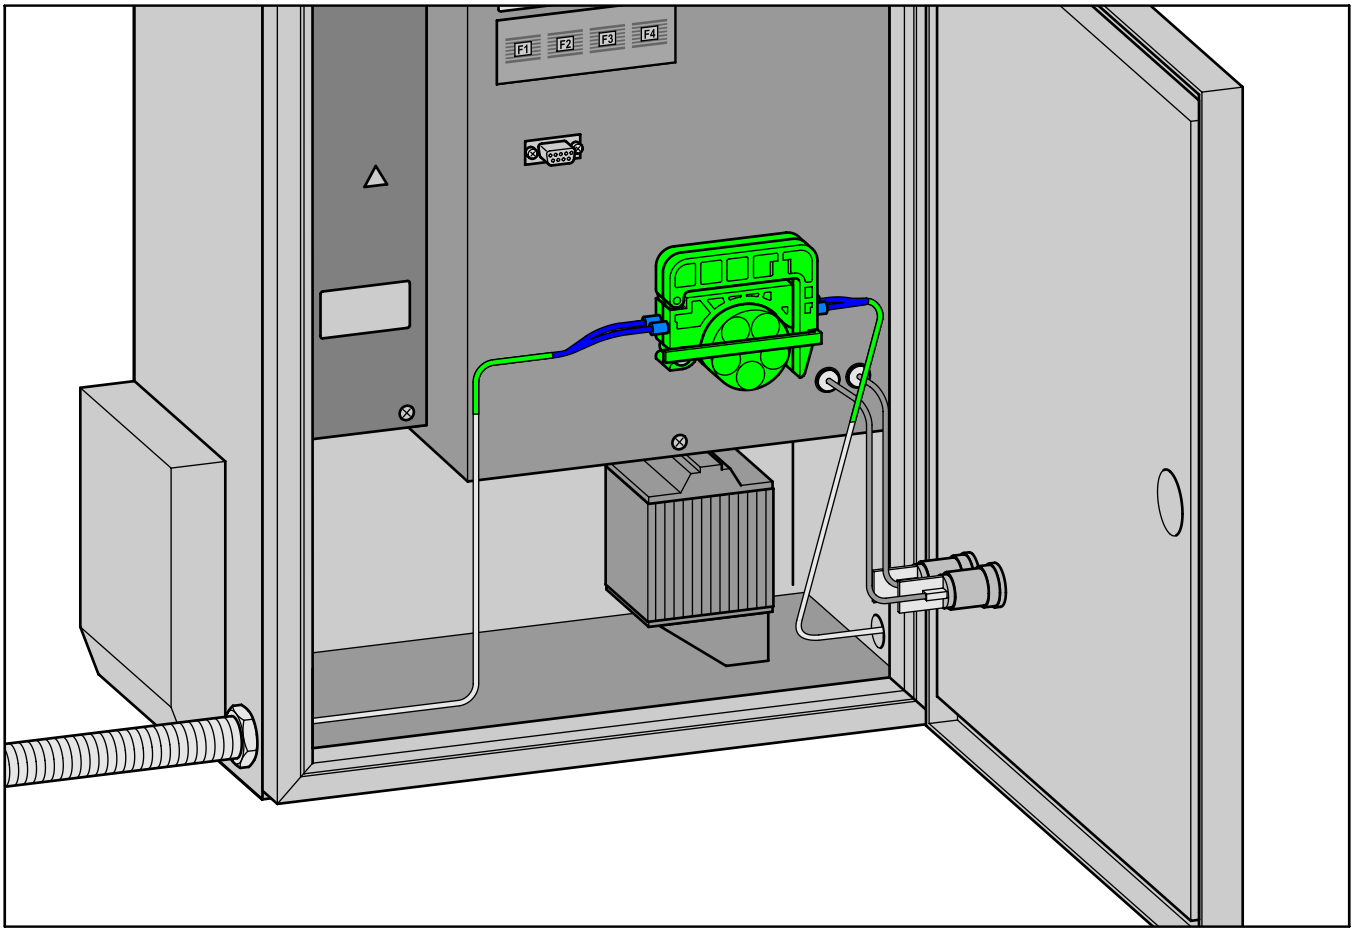
Every 12 month
Replace
- Pump Cartridges
- Pump Rollers
- Connecting Tubes

Every 6 month
Check
- Pump Cartridges
- Pump Rollers
- Filter Module
- Connecting Tubes
- Elektronics

Every 3 month
Replace
- Pump Tubes
- Air Filter (Control Unit)

Clean
- Filter Module (if/as necessary)
- Sample Tubes (if/as necessary)

Weekly
Visual Inspection
- Sample Quality
- Device Function
- Air Filter (Control Unit)


F1
F2
F3
F4

