

Chloramine (Mono) and Nitrogen, Free Ammonia

DOC316.53.01016

Indophenol Method¹**Method 10200****0.04 to 4.50 mg/L Cl₂****Powder Pillows****0.01 to 0.50 mg/L NH₃-N**

Scope and application: For the determination of free ammonia and monochloramine simultaneously in finished chloraminated water. This product has not been evaluated to test for chlorine and chloramines in medical applications in the United States.

¹ U.S. Patent 6,315,950





Test preparation

Instrument-specific information

Table 1 shows all of the instruments that have the program for this test. The table also shows requirements that can change between instruments, such as adapter and sample cell requirements.

To use the table, select an instrument, then read across to find the applicable information for this test.

Table 1 Instrument-specific information

Instrument	Adapter	Sample cell orientation	Sample cell
DR6000	—	The orientation key is toward the arrow on the universal cell adapter.	 4864302
DR5000	A23618	The orientation key is toward the user.	
DR3900	LZV846 (A)	The orientation key is away from the user.	
DR1900	9609900 or 9609800 (C)	The orientation key is toward the arrow on the adapter.	
DR/850, DR/890	—	The orientation key is at the 2 o'clock position.	
DR900	—	The orientation key is toward the user.	
DR3800 DR2800 DR2700	LZV585 (B)	The 1-cm path is aligned with the arrow on the adapter.	 5940506

Before starting

Samples must be analyzed immediately after collection and cannot be preserved for later analysis.

Install the instrument cap on the DR900 and DR800 series cell holder before ZERO or READ is pushed.

In bright light conditions (e.g., direct sunlight), close the cell compartment, if applicable, with the protective cover during measurements.

For the best results, measure the reagent blank value for each new lot of reagent. Replace the sample with deionized water in the test procedure to determine the reagent blank value. Subtract the reagent blank value from the sample results automatically with the reagent blank adjust option.

Review the Safety Data Sheets (MSDS/SDS) for the chemicals that are used. Use the recommended personal protective equipment.

Dispose of reacted solutions according to local, state and federal regulations. Refer to the Safety Data Sheets for disposal information for unused reagents. Refer to the environmental, health and safety staff for your facility and/or local regulatory agencies for further disposal information.

Items to collect


Description	Quantity
Free Ammonia Chlorinating Solution	1 drop
Monochlor F Reagent Pillows	2
Sample cells (For information about sample cells, adapters or light shields, refer to Instrument-specific information on page 1.)	2

Refer to [Consumables and replacement items](#) on page 8 for order information.


Sample collection and storage

- Analyze samples immediately after collection.
- Collect samples in clean glass bottles.
- Open the sample valve or spigot and let the water flow for a minimum of 5 minutes.
- Rinse the sample bottle several times with the sample and let the sample overflow each time, then cap the container so that there is no head space (air) above the sample.


Powder pillow procedure

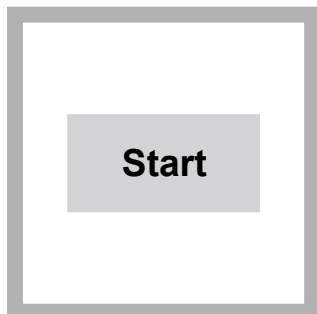


1. For the DR 800 series, enter and start program **132**.

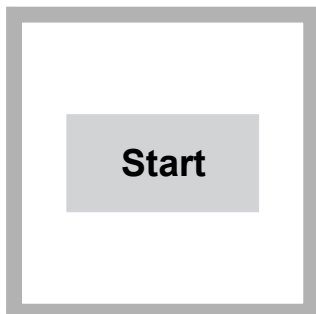


2. For other instruments, start program **66**, **Monochloramine LR**. For information about sample cells, adapters or light shields, refer to [Instrument-specific information](#) on page 1.

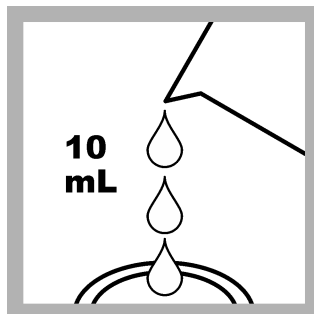


3. Fill two sample cells to the 10-mL line with sample. Write **Free Ammonia** on one sample cell. Write **Monochloramine** on the second sample cell.

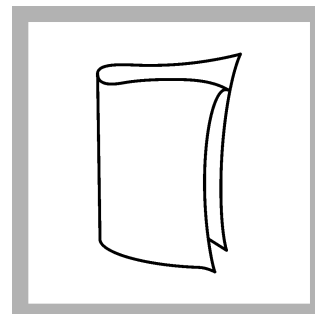


4. Clean the **monochloramine** sample cell.

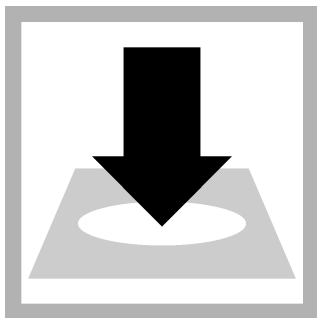

5. Insert the **monochloramine** sample cell into the cell holder.

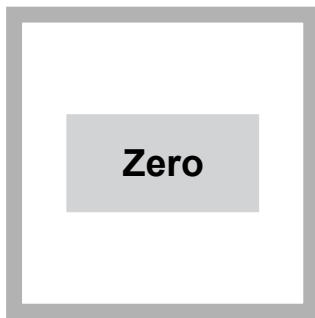


6. Push **ZERO**. The display shows 0.00 mg/L Cl_2 .

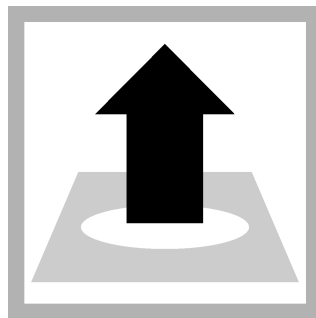

7. Remove the sample cell from the cell holder.




8. Add **one** drop of Free Ammonia Chlorinating Solution to the sample cell for **free ammonia** measurement. Close the reagent bottle to keep the reagent stable.

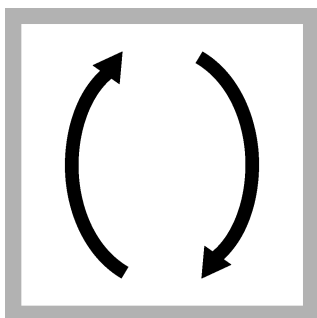


9. Close the **free ammonia** sample cell. Invert the sample cell to mix the reagent for 15 seconds.



10. Start the instrument timer. A 1-minute reaction time starts. If the sample pH is more than 9.5, increase the reaction time to 2 minutes. If the sample becomes cloudy by the end of the reaction period, pretreat the sample and start over. Refer to [Interferences](#) on page 5.

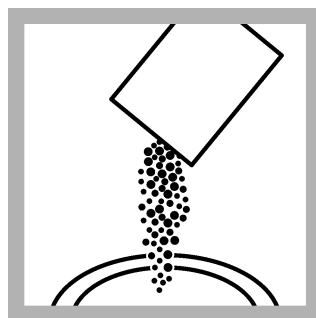


11. Add the contents of one Monochlor F Reagent Powder Pillow to each sample cell.

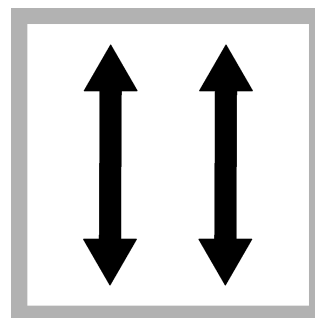


12. Put the stoppers on the sample cells. Shake the sample cells for about **20 seconds** to dissolve the reagent. A green color will show if monochloramine or free ammonia is present.




13. Start the instrument timer. A 5-minute reaction time starts. For samples colder than 18 °C, refer to [Table 2](#) on page 4.

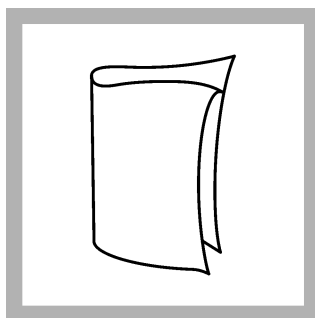


14. When the timer expires, clean the **monochloramine** sample cell. Make sure that there are no air bubbles in the sample cell after the reaction. If there are bubbles, invert the sample cell to remove the bubbles.

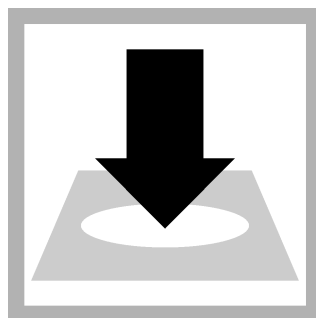


15. Insert the **monochloramine** sample cell into the cell holder.

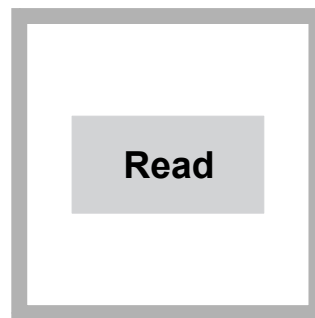


16. Push **READ**. Results show in mg/L Cl_2 .

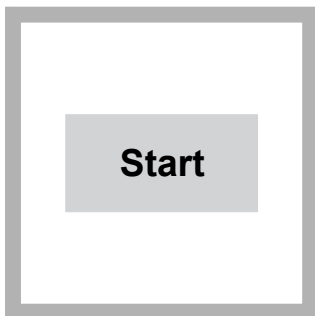


17. For the DR 800 series, exit program 132. Start program 133.

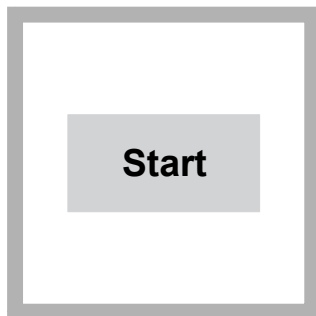


18. For other instruments, exit program 66. Start program 389 N, Ammonia Free.

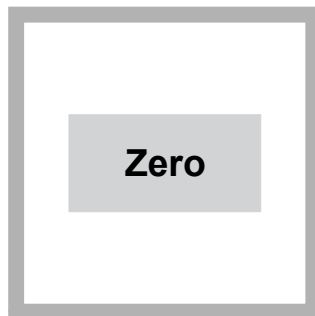


19. Leave the **monochloramine** sample cell in the cell holder. Push **ZERO**. The display will show 0.00 mg/L NH₃-N f.

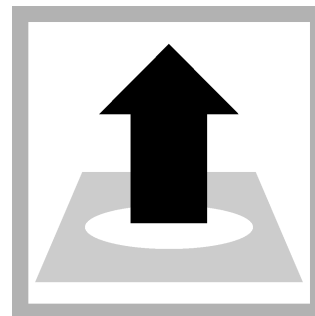


20. Remove the monochloramine sample cell from the cell holder.

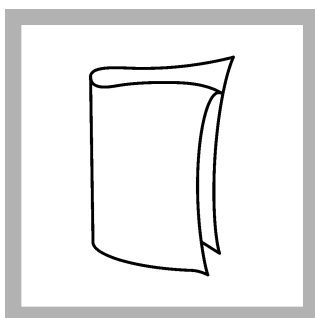

21. Clean the **free ammonia** sample cell. Make sure that there are no air bubbles in the sample cell after the reaction. If there air bubbles, invert the cell to remove the bubbles.

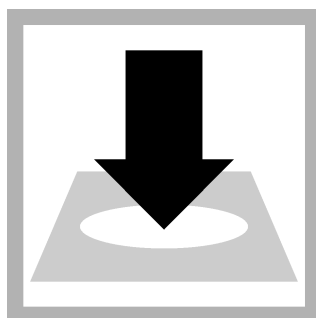

22. Insert the **free ammonia** sample cell into the cell holder.

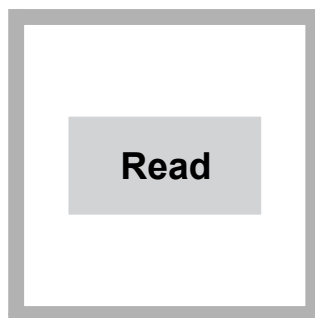

23. Push **READ**. The results are in mg/L NH₃-N f.

Color development time

Test results are strongly influenced by the sample temperature. The reaction times in the procedure are for samples at 18–20 °C (64–68 °F). Adjust the reaction times for the sample temperature as shown in [Table 2](#). The color is stable for a maximum of 15 minutes after the specified development time.

If the sample temperature is less than 10 °C (50 °F), especially if the sample is measured outdoors in cold weather, measure the prepared sample again 5 to 10 minutes after the development time given in [Table 2](#). Measure the prepared sample again to make sure that the reaction has completed. The colorimetric reaction has completed if the results do not increase by more than 10% within 10 minutes of the development time.

Table 2 Color development time

Sample temperature (°C)	Sample temperature (°F)	Development time (minutes)
5	41	10
7	45	9
9	47	8
10	50	8
12	54	7
14	57	7
16	61	6

Table 2 Color development time (continued)

Sample temperature (°C)	Sample temperature (°F)	Development time (minutes)
18	64	5
20	68	5
23	73	2.5
25	77	2
> 25	> 77	2

Interferences

This method is intended for finished, chloraminated drinking water samples that have a measurable combined (total) chlorine disinfectant residual. Samples that do not have a disinfectant residual and samples that have a chlorine demand can cause low ammonia test results. Blanks and ammonia standards that are analyzed without a disinfectant residual must be prepared with high quality, reagent grade water.

The substances that are shown in [Table 3](#) do not interfere in the free ammonia determination at or below the given concentration.

Table 3 Non-interfering substances

Substance	Maximum level tested
Al	0.2 mg/L
Cl ⁻	1200 mg/L
Cu	1 mg/L
Fe	0.3 mg/L
Mn	0.05 mg/L
NO ₃ ⁻ -N	10 mg/L
NO ₂ ⁻ -N	1 mg/L
PO ₄ ³⁻	70 mg/L
SiO ₂	100 mg/L
SO ₄ ²⁻	1600 mg/L
Zn	5 mg/L

Samples that contain high levels of both total hardness and alkalinity may become cloudy after the addition of the Free Ammonia Chlorinating Solution. If this occurs by the end of the first reaction period, the sample for Free Ammonia measurement must be pretreated as follows:

1. Measure 10 mL of sample into the sample cell for Free Ammonia.
2. Add the contents of one Hardness Treatment Reagent Powder Pillow to the sample.
3. Tighten the cap on the sample cell and invert until the reagent is dissolved.
4. Remove the cap.
5. Use the pretreated sample in the test procedure for the Free Ammonia sample.

For samples with a pH less than 8, monochloramine may not form after Free Ammonia Chlorinating Solution is added. If this occurs, add one drop of 1 N Sodium Hydroxide Standard Solution to the sample before Free Ammonia Chlorinating Solution is added. The addition of Sodium Hydroxide Standard Solution increases the pH to appropriate levels to form monochloramine.

Note: *The sample for Monochloramine measurement does not need pretreatment.*

Accuracy check

Standard solution method

Items to collect:

- Buffer Powder Pillow, pH 8.3
- Nitrogen, Ammonia Standard Solution, 100 mg/L as $\text{NH}_3\text{-N}$
- Chlorine Solution Ampules, 50–70 mg/L
- 100-mL Class A volumetric flask
- 50-mL graduated cylinder
- Pipet, TenSette®, 0.1–1.0 mL and tips
- Pipets, Volumetric, 2 mL Class A and Mohr, 5 mL
- Pipet bulb
- Organic-free water

1. Prepare a 4.5-mg/L (as Cl_2) monochloramine standard immediately before use as follows.
 - a. Add the contents of one Buffer Powder Pillow, pH 8.3 to approximately 50 mL of organic-free water in a clean 100-mL Class A volumetric flask. Swirl to dissolve the powder.
 - b. Use a Class A volumetric pipet to add 2.00 mL of Nitrogen, Ammonia Standard Solution, 100 mg/L as $\text{NH}_3\text{-N}$ into the flask.
 - c. Dilute to the mark with organic-free water. Mix well. This is a 2.00-mg/L buffered ammonia standard.
 - d. Use a graduated cylinder to add 50.00 mL of the buffered ammonia standard into a clean 100-mL beaker. Add a stir bar.
 - e. Find the exact concentration of the Chlorine Solution Ampules, 50–70 mg/L from the label on the package.
 - f. Calculate the volume of the Chlorine Solution to add to the ammonia standard:
mL chlorine solution required = $455/(\text{free chlorine concentration})$.
 - g. Open an ampule and use a glass Mohr pipet to add the calculated amount of Chlorine Solution slowly to the ammonia standard in the beaker. Keep the beaker on a stir-plate at medium speed during the chlorine addition.
 - h. Stir the monochloramine solution for 1 minute after the Chlorine Solution addition is complete.
 - i. Quantitatively transfer the monochloramine solution to a clean 100-mL Class A volumetric flask. Dilute to the mark with organic-free water and mix well. This is a nominal 4.5-mg/L (as Cl_2) monochloramine standard.
2. Use this standard within 1 hour of preparation. Use the test procedure to measure the concentration of the monochloramine standard solution.
3. Compare the expected result to the actual result.

Note: The factory calibration can be adjusted slightly with the standard calibration adjust option so that the instrument shows the expected value of the standard solution. The adjusted calibration is then used for all test results. This adjustment can increase the test accuracy when there are small variations in the reagents or instruments.

Standard additions method (sample spike)

Use the standard additions method (for applicable instruments) to validate the test procedure, reagents and instrument and to find if there is an interference in the sample.

Items to collect:

- Ammonium Nitrogen Standard Solution, 10 mg/L $\text{NH}_3\text{-N}$
- 50-mL mixing cylinders
- Pipet, TenSette®, 0.1–1.0 mL and tips

1. Use the test procedure to measure the concentration of the sample, then keep the (unspiked) sample in the instrument.
2. Go to the Standard Additions option in the instrument menu.
3. Select the values for standard concentration, sample volume and spike volumes.
4. Open the standard solution.
5. Prepare three spiked samples: use the TenSette pipet to add 0.3 mL, 0.6 mL and 1.0 mL of the standard solution, respectively, to three 50-mL portions of fresh sample. Mix well.
6. Use the test procedure to measure the concentration of each of the spiked samples. Start with the smallest sample spike. Measure each of the spiked samples in the instrument.
7. Select **Graph** to compare the expected results to the actual results.

Note: If the actual results are significantly different from the expected results, make sure that the sample volumes and sample spikes are measured accurately. The sample volumes and sample spikes that are used should agree with the selections in the standard additions menu. If the results are not within acceptable limits, the sample may contain an interference.

Standard solution method

Use the standard solution method to validate the test procedure, the reagents and the instrument.

Items to collect:

- Ammonium Nitrogen Standard Solution, 10 mg/L NH₃-N
- 100-mL plastic volumetric flask with stopper, Class A
- 2-mL volumetric pipet, Class A and pipet filler safety bulb
- Deionized water—must be free of ammonia, chlorine and chlorine demand, for example 18 MΩ-cm water from a deionizer system.

1. Prepare a 0.20 mg/L ammonia nitrogen standard solution as follows:
 - a. Use a pipet to add 2.00 mL of 10 mg/L ammonia nitrogen standard solution into the volumetric flask. (Alternate preparation: add 0.4 mL of a 50 mg/L ammonia nitrogen standard solution to the volumetric flask.)
 - b. Dilute to the mark with deionized water. Mix well. Prepare this solution daily.
2. Use the test procedure to measure the concentration of the prepared standard solution.
3. Compare the expected result to the actual result.

Note: The factory calibration can be adjusted slightly with the standard calibration adjust option so that the instrument shows the expected value of the standard solution. The adjusted calibration is then used for all test results. This adjustment can increase the test accuracy when there are small variations in the reagents or instruments.

Method performance

The method performance data that follows was derived from laboratory tests that were measured on a spectrophotometer during ideal test conditions. Users can get different results under different test conditions.

Program	Standard	Precision (95% Confidence Interval)	Sensitivity Concentration change per 0.010 Abs change
66	2.60 mg/L Cl ₂	2.58–2.62 mg/L Cl ₂	0.04 mg/L Cl ₂
389	0.20 mg/L NH ₃ -N	0.19–0.21 mg/L NH ₃ -N	0.01 mg/L NH ₃ -N

Summary of method

Monochloramine (NH₂Cl) and free ammonia (NH₃ and NH₄⁺) can exist in the same water sample. Added hypochlorite combines with free ammonia to form more monochloramine. In the presence of a cyanoferrate catalyst, monochloramine in the sample reacts with a substituted phenol to form an intermediate monoimine compound. The intermediate

couples with excess substituted phenol to form a green-colored indophenol, which is proportional to the amount of monochloramine present in the sample. Free ammonia is determined by comparing the color intensities, with and without added hypochlorite. The measurement wavelength is 655 nm for spectrophotometers or 610 nm for colorimeters.

Consumables and replacement items

Required reagents

Description	Quantity/test	Unit	Item no.
Free Ammonia Reagent Set, includes:	—	50/pkg	2879200
Free Ammonia Chlorinating Solution	1 drop	4 mL SCDB	2877436
Monochlor F Reagent Pillows	2	100/pkg	2802299

Recommended standards and apparatus

Description	Unit	Item no.
Buffer Powder Pillows, pH 8.3	25/pkg	89868
Chlorine Standard Solution, 10-mL Voluette [®] Ampule, 50-75 mg/L	16/pkg	1426810
Chlorine Standard Solution, 2-mL PourRite [®] Ampule, 50-75 mg/L	20/pkg	1426820
Chlorine Standard Solution, 2-mL PourRite [®] Ampules, 25-30 mg/L	20/pkg	2630020
Hardness Treatment Reagent Pillows	50/pkg	2882346
Nitrogen Ammonia Standard Solution, 10-mg/L NH ₃ -N	500 mL	15349
Nitrogen Ammonia Standard Solution, 10-mL Voluette [®] Ampule, 50-mg/L NH ₃ -N	16/pkg	1479110
Nitrogen Ammonia Standard Solution, 100-mg/L as NH ₃ -N	500 mL	2406549
PourRite [®] Ampule Breaker, 2 mL	each	2484600
Ampule Breaker, 10-mL Voluette [®] Ampules	each	2196800
Water, organic-free	500 mL	2641549

Optional reagents and apparatus

Description	Unit	Item no.
Beaker, 100 mL, polypropylene	each	108042
Beaker, glass, 100 mL	each	50042H
Mixing cylinder, graduated, 50 mL	each	2088641
Flask, volumetric, Class A, 100 mL, glass	each	1457442
Monochloramine/Free Ammonia SpecCheck [™] Kit	each	2507500
Pipet filler, safety bulb	each	1465100
Pipet, TenSette [®] , 0.1-1.0 mL	each	1970001
Pipet tips for TenSette [®] Pipet, 0.1-1.0 mL	50/pkg	2185696
Pipet tips for TenSette [®] Pipet, 0.1-1.0 mL	1000/pkg	2185628
Pipet, Mohr, glass, 10 mL	each	2093438
Pipet, volumetric, Class A, 2 mL	each	1451536
Pipet, volumetric, Class A, 50 mL	each	1451541
Scissors	each	2883100
Sodium Hydroxide Standard Solution, 1.00 N	100 mL MDB	104532

Optional reagents and apparatus (continued)

Description	Unit	Item no.
Stir bar, octagonal	each	2095352
Stirrer, magnetic	each	2881200
Thermometer, -10 to 110 °C	each	187701
Wipes, disposable	280/pkg	2097000



FOR TECHNICAL ASSISTANCE, PRICE INFORMATION AND ORDERING:
In the U.S.A. – Call toll-free 800-227-4224
Outside the U.S.A. – Contact the HACH office or distributor serving you.
On the Worldwide Web – www.hach.com; E-mail – techhelp@hach.com

HACH COMPANY
WORLD HEADQUARTERS
Telephone: (970) 669-3050
FAX: (970) 669-2932