


**Certificate of Analysis
 Technical Data for Validation of
 COD Digestion Vials
 (20 – 1500 mg/L)**

The data for this Certificate of Analysis follows the procedures in USEPA Approved Hach Method 8000 and ISO 8466.

Catalog Number	2125915
Date of Certificate	January 16, 2015
Number of Lots	50

Sensitivity (0.010 Abs Change)	23 mg/L COD
Reagent Blank	3.3 mg/L COD
Accuracy	3.1 %
Vial to Vial Variability	2.4 mg/L COD
Confidence Interval (95%)	0.22 %
Method Standard Deviation	12 mg/L COD
Method Variation Coefficient	0.9 %
Detection Limit	4.0 mg/L COD
Quantitation Limit	13 mg/L COD

Expected Value mg/L COD	Average Obtained Value mg/L COD
1200	1237

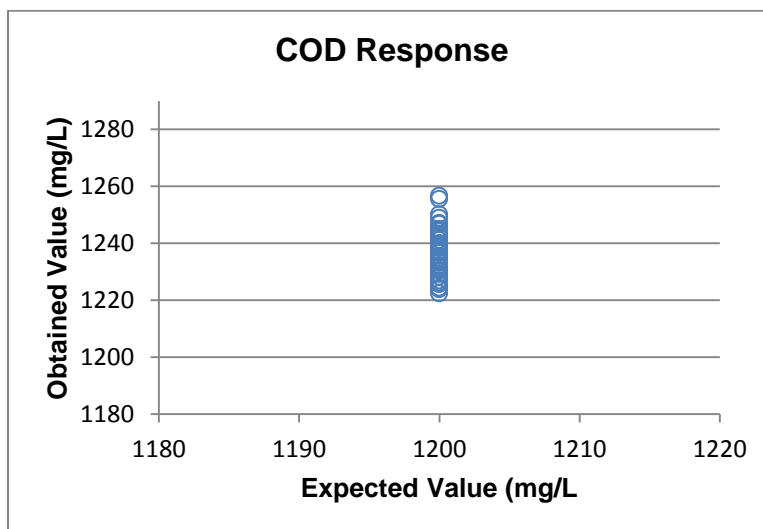

Scott Als, Quality Chemist

Scott Als

